

FIGURE 1

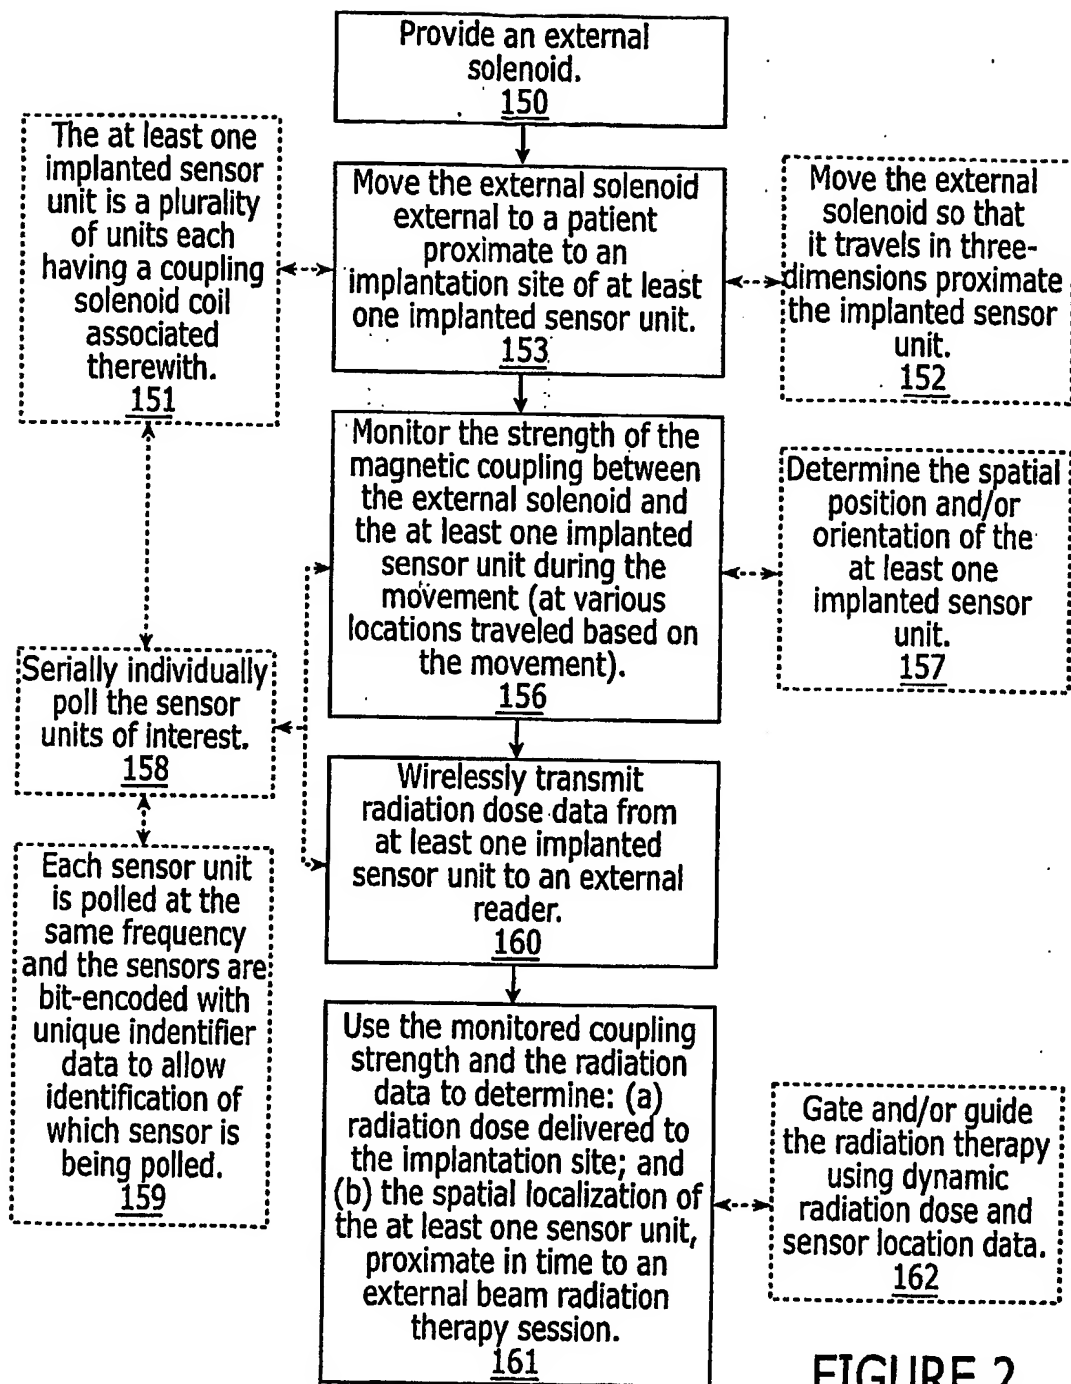


FIGURE 2

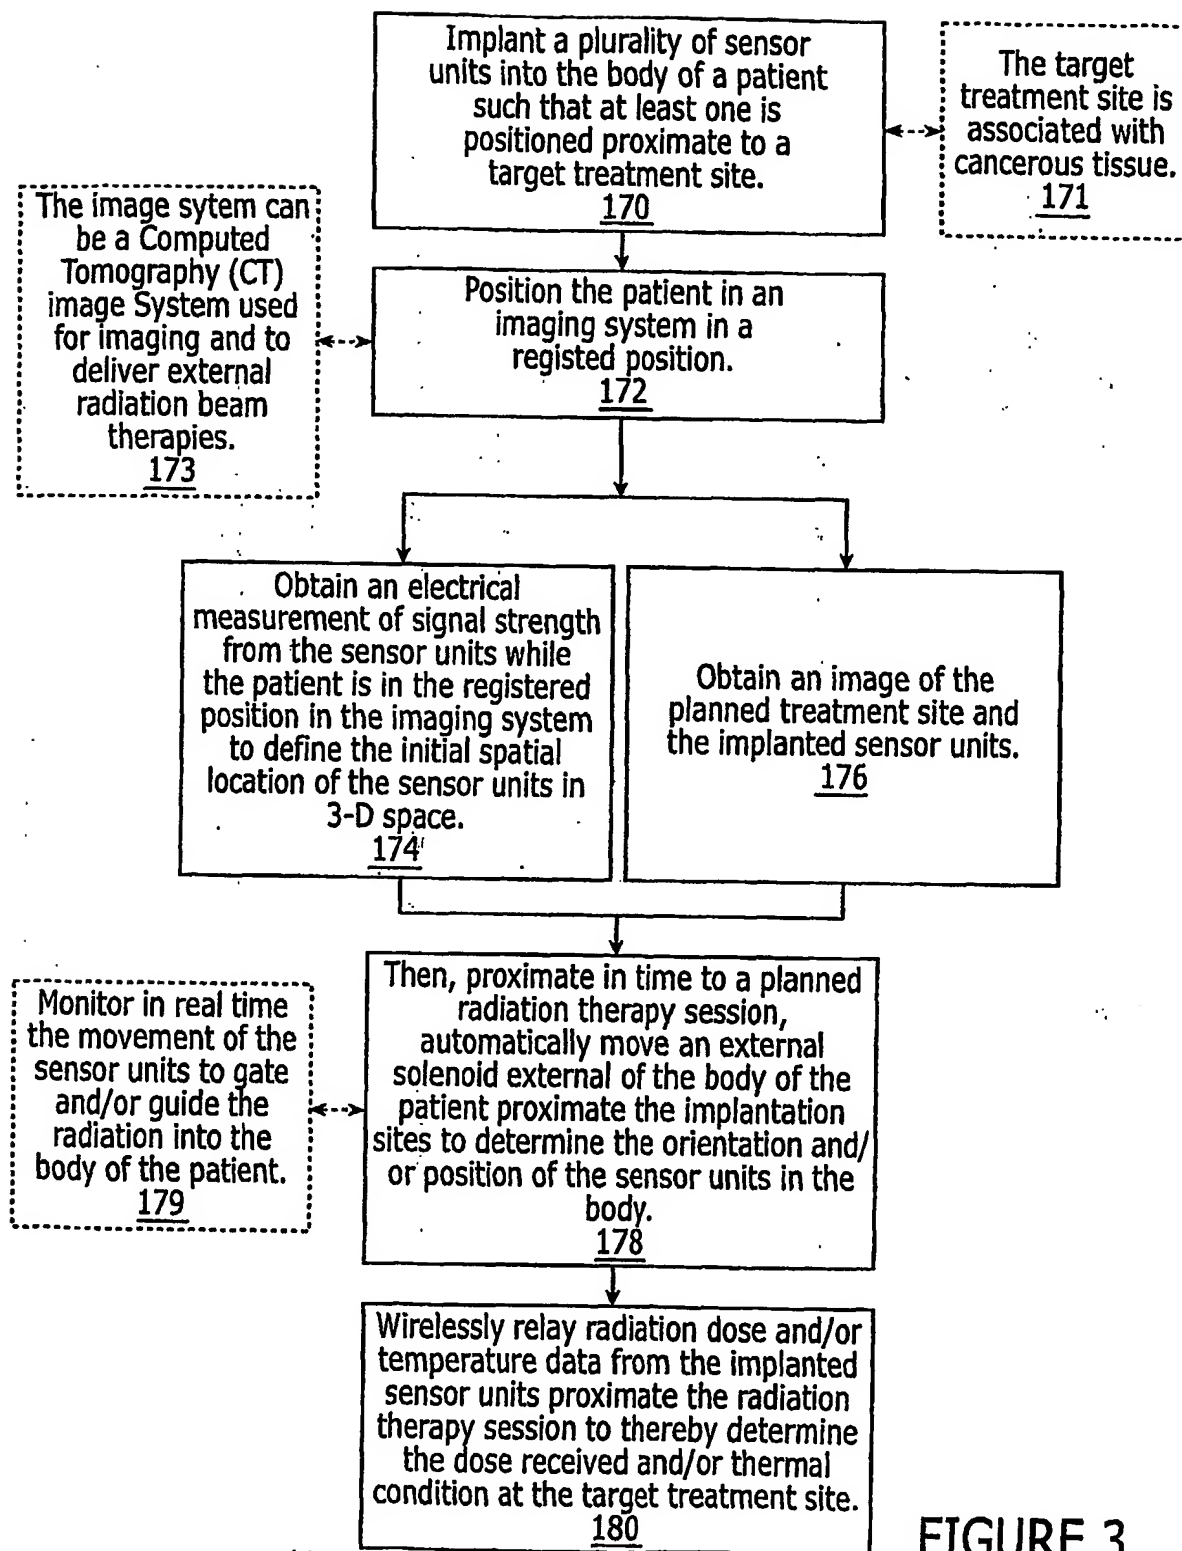


FIGURE 3

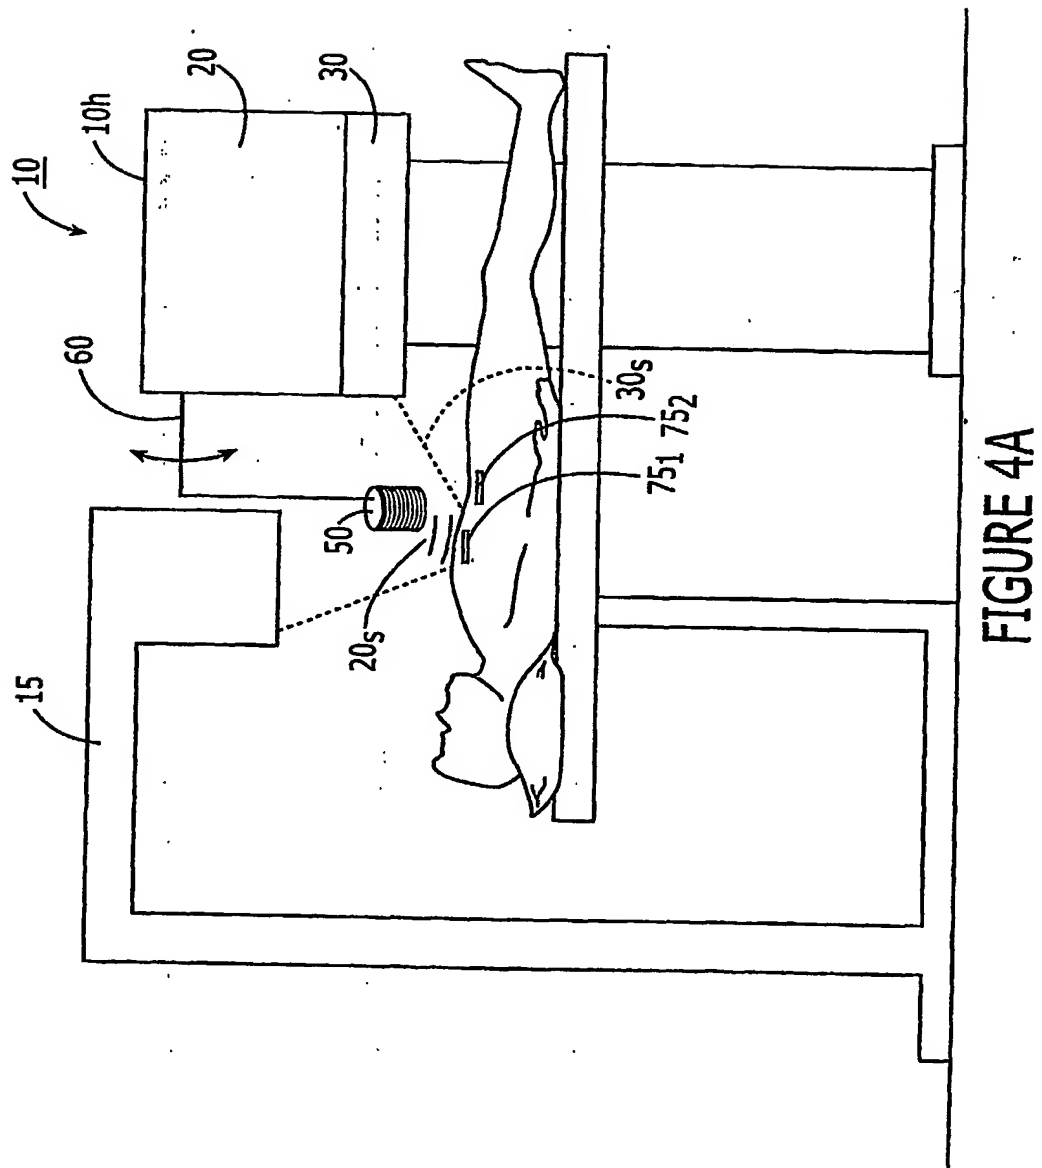


FIGURE 4A





FIGURE 4B

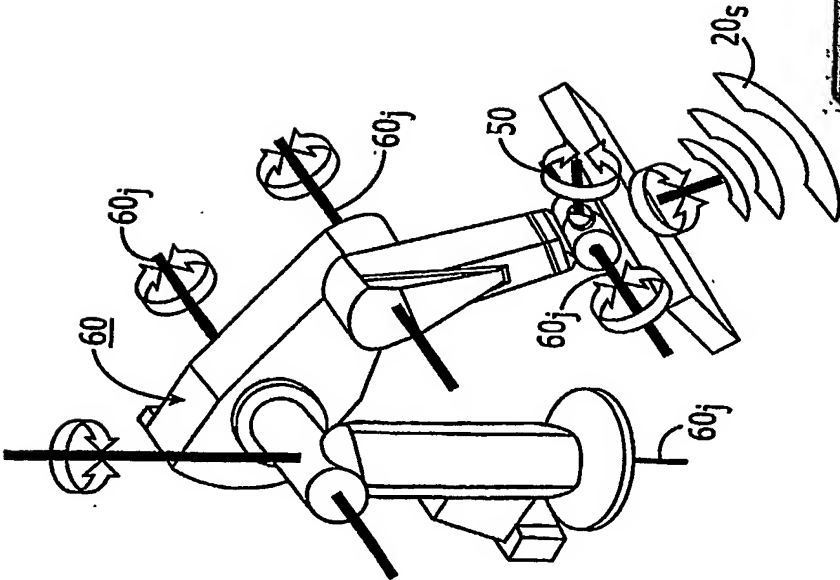

- Real-time positional tracking
- Temperature data for hyperthermia/radiation combination therapy


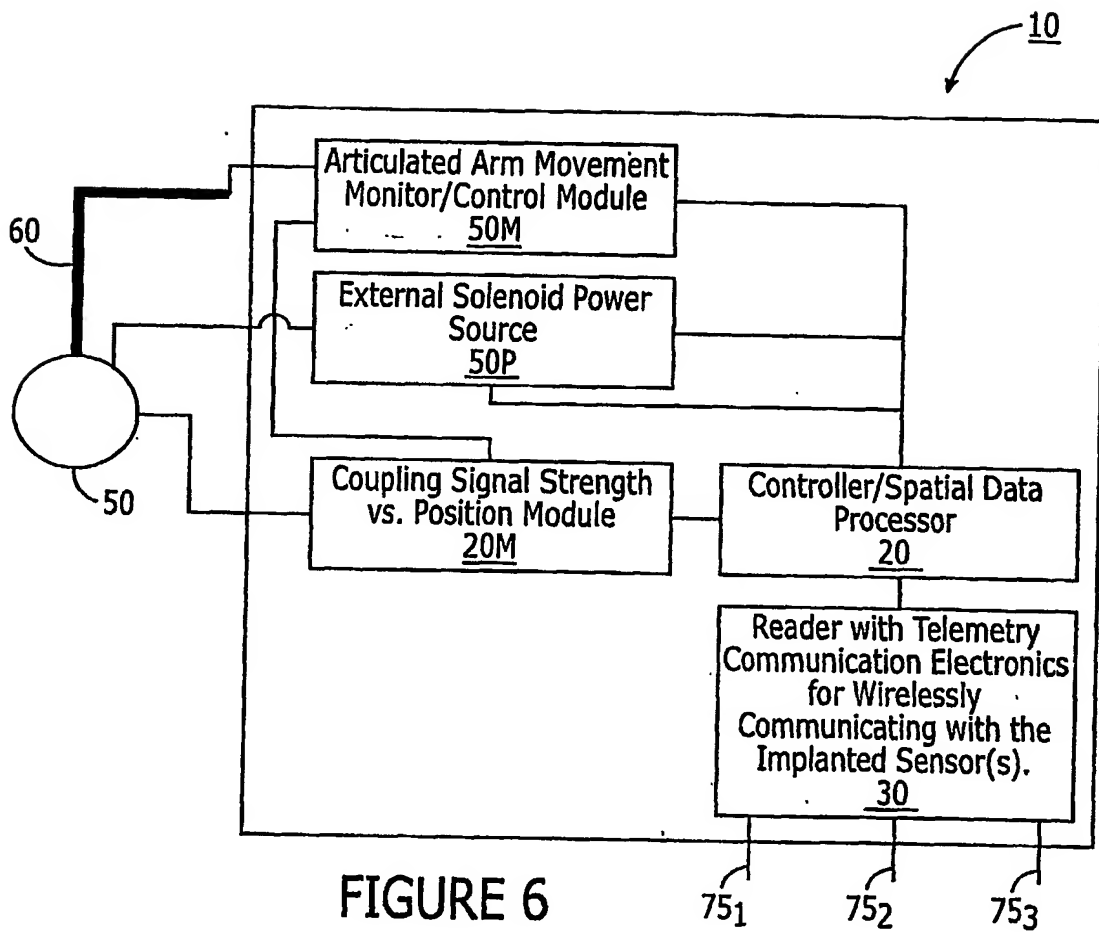


FIGURE 5





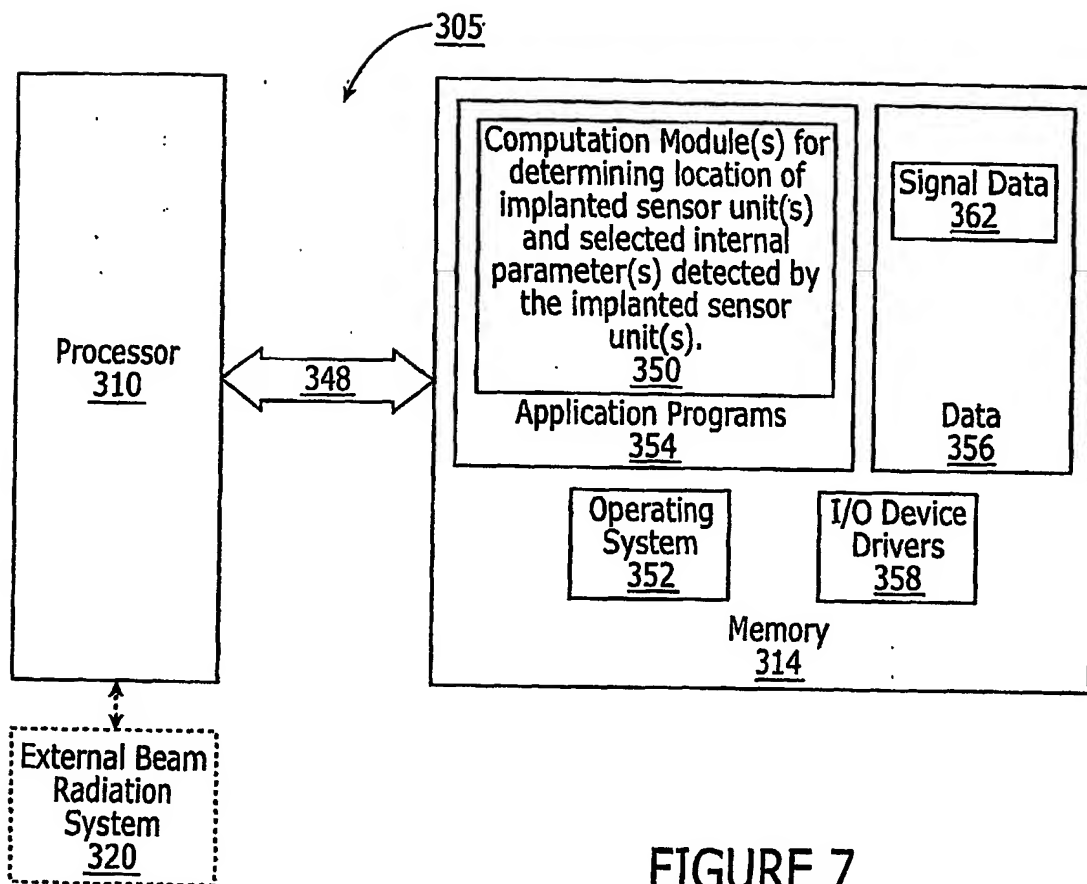


FIGURE 7



BEST AVAILABLE COPY

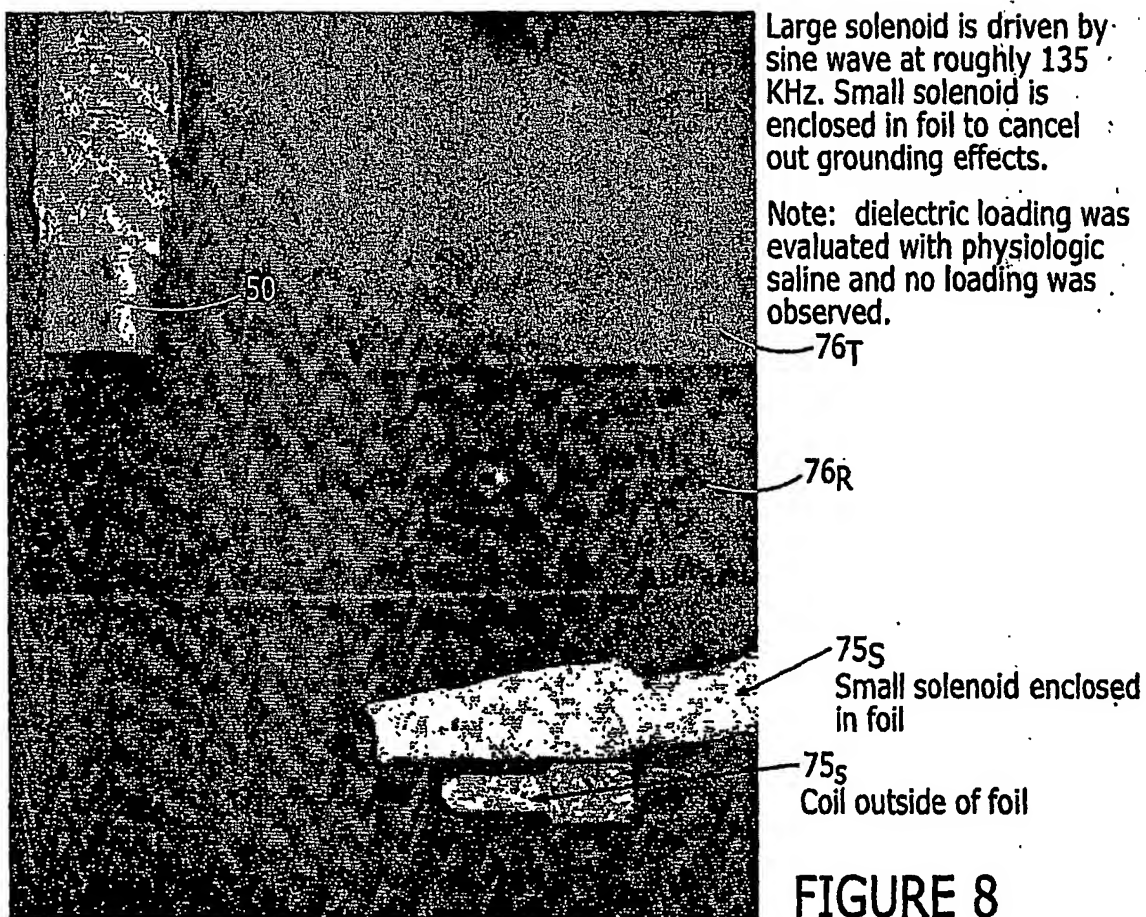

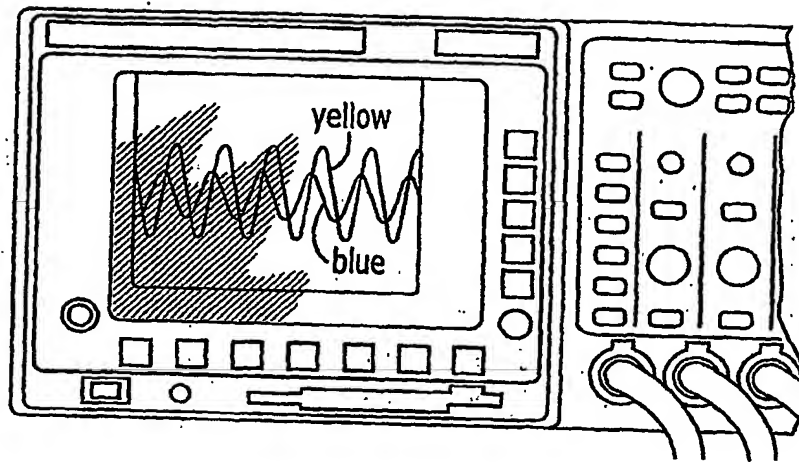

Applied voltage (yellow) to large solenoid and response voltage (blue) of small solenoid. Frequency was adjusted to achieve maximum coupling.

FIGURE 9


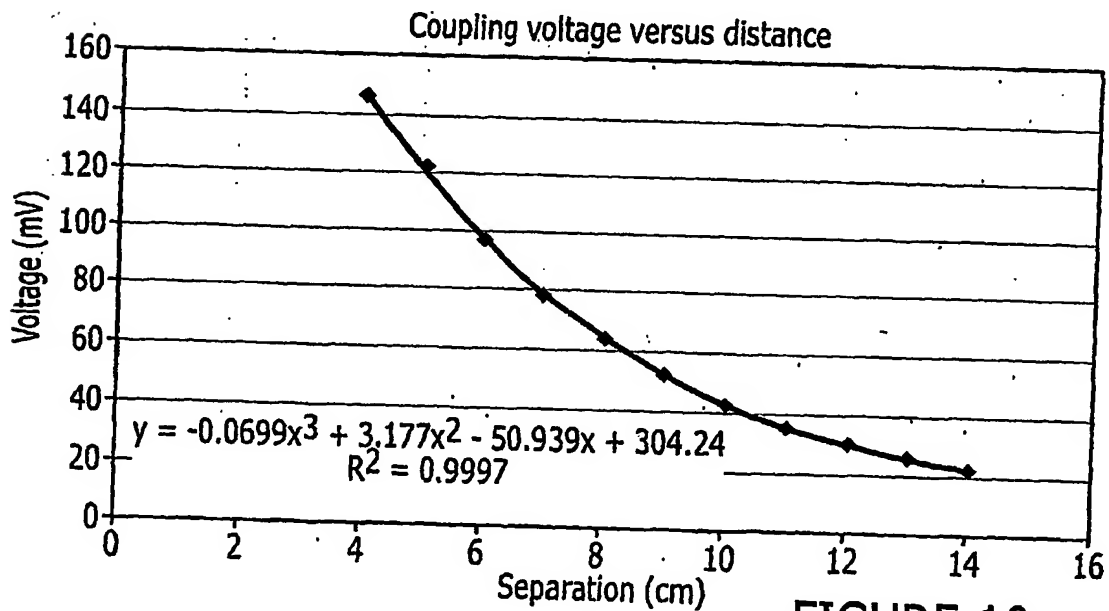


FIGURE 10

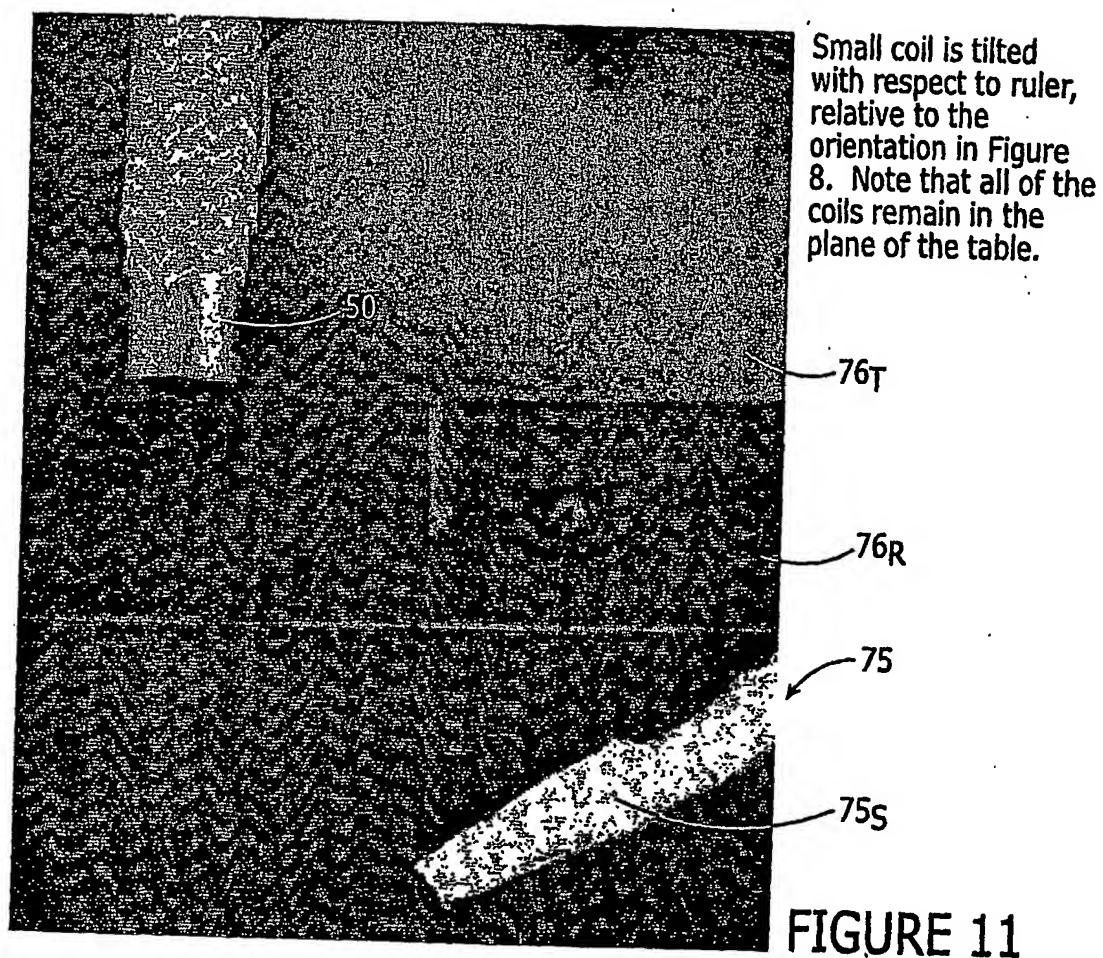

BEST AVAILABLE COPY

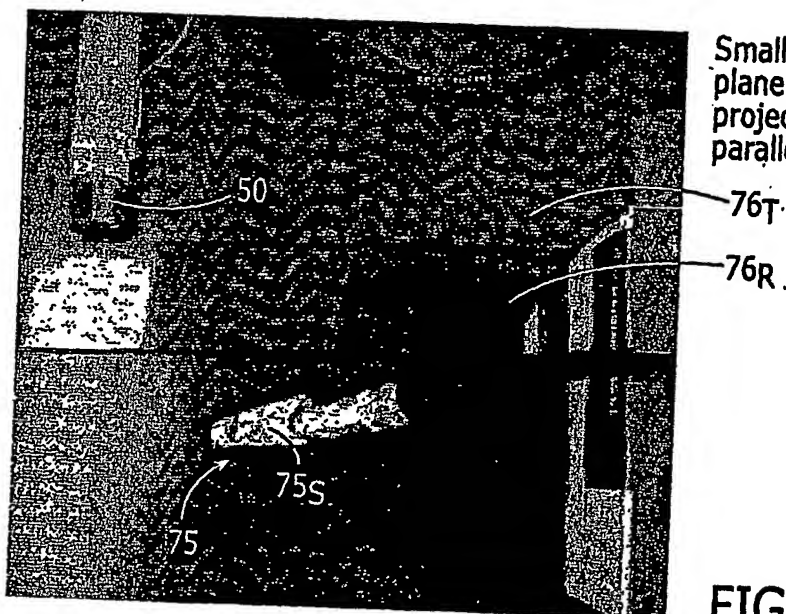


FIGURE 12

BEST AVAILABLE COPY